# **BPAP System Y / U Series Quick Operation Manual**


## 1. Button Functions

Mute Button: Press it to mute the alert

Knob: Start treatment and adjust device settings

Ramp Button: Press it to enable the Ramp feature

# 2. Setting up the Device

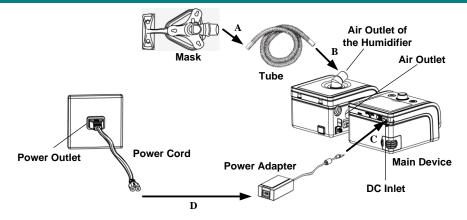

- A. Connect one end of the tube to the assembled mask.
- B. Connect the other end of the tube securely to the air outlet of the main device or of the humidifier, as shown in the figure above.
- C. Connect the power adapter to the DC inlet of the main device.
- D. Connect the power cord to the power adapter.
- E. Plug the power cord into the power outlet.


#### 3. Adjusting Device Settings

A. After the device is connected to power, its screen displays the Main Interface shown in the first figure below, or the Main Interface shown in the second figure below.

Note: The value of blood oxygen saturation (SpO<sub>2</sub>) and pulse rate can only be seen after the SpO<sub>2</sub> Kit is connected to the main device correctly.





The above interface only applies to U-20T, U-25T, U-30T, U-30AT.



The above interface only applies to Y-20T, Y-25T, Y-30T, Y-30AT.

B. From the Main Interface shown above, press and hold **the Ramp Button**  $\triangle$  for three seconds. The screen displays the Initial Setup Interface, as shown in the figure below.



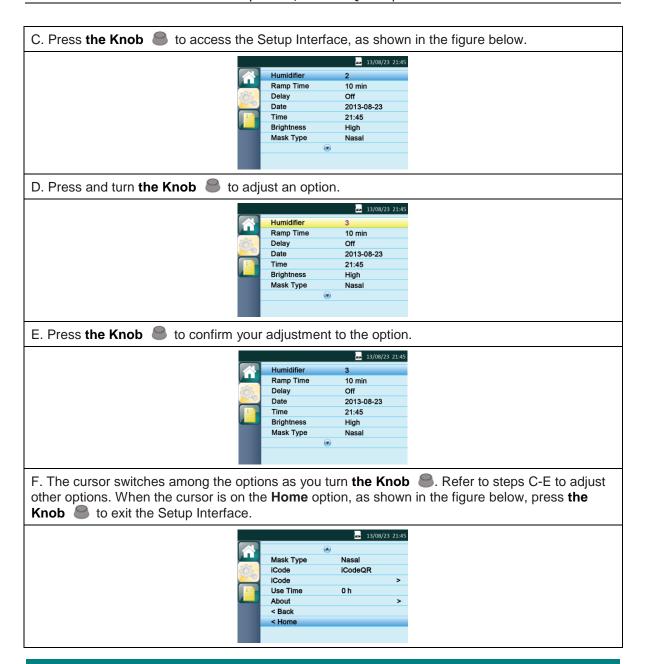

## 4. Starting Treatment

After you finish adjusting device settings and return to the Main Interface, press **the Knob** to start treatment.

# 5. Important Tips

Please refer to the user manual for any information on the use of the SpO<sub>2</sub> Kit and SD card.

Before using the device, please read the entire user manual and memorize all information necessary to ensure proper use of the device.